INTEGRATED POWER DESIGNS

300 Stewart Road
Wilkes-Barre, PA 18706 USA
Phone: (570) 824-4666

Web: www.ipdpower.com
Email: sales@ipdpower.com
Fax: (570) 824-4843

DC1-80 SERIES OPERATING INSTRUCTIONS

INPUT RATING: 9-18VDC, 15A

OUTPUT RATING: 80 Watts Max. Output Power with 300 LFM Forced Air. Open Frame or with Chassis.
60 Watts Max. Output Power Convection Cooled. Open Frame or with Chassis. Single Outputs.
50 Watts Max. Output Power Convection Cooled. Open Frame or with Chassis. Multi Outputs.

MODEL LISTING:

MODEL	OUTPUT 1	OUTPUT 2	OUTPUT 3	OUTPUT 4
DC1-80-4001	+3.3V/6A	+5V/5A	+12V/2A	-12V/2A
DC1-80-4002	+5V/6A	+3.3V/5A	+12V/2A	-12V/2A
DC1-80-4003	+5V/6A	-5V/5A	+12V/2A	-12V/2A
DC1-80-4004	+5V/6A	-5V/5A	+15V/2A	-15V/2A
DC1-80-4005	+5V/6A	+24V/2A	+12V/2A	-12V/2A
DC1-80-4006	+5V/6A	+24V/2A	+15V/2A	-15V/2A
DC1-80-3001	+5V/6A	+12V/2A		-12V/2A
DC1-80-3002	+5V/6A	+15V/2A		-15V/2A
DC1-80-2001	+5V/6A	+12V/4A		
DC1-80-2002	+5V/6A	+24V/2A		
DC1-80-2003	+12V/3.5A	-12V/3.5A		
DC1-80-2004	+15V/3A	-15V/3A		
DC1-80-1001	5V/16A			
DC1-80-1002	12V/6.7A			
DC1-80-1003	15V/5.3A			
DC1-80-1004	24V/3.3A			
DC1-80-1005	28V/2.9A			
DC1-80-1006	36V/2.2A			
DC1-80-1007	48V/1.7A			
DC1-80-1008[2]	19V/4.2A			

NOTES:
1. A suffix may be added to the model number to indicate the following optional configurations: (CH-chassis, IO-isolated outputs, TS-terminal strip).
2. Approved to EN 60601-1:2006/A2:2021 and IEC 60601-1:2005/A2:2020 only.

DECLARATION OF CONFORMITY

Manufacturer: Integrated Power Designs, Inc.
Manufacturer's Address: 300 Stewart Road, Wilkes-Barre, PA 18706 USA
Product Type: Switchmode DC-DC Power Supply

Declares all models listed above including all options are in compliance with the following European Community Directives:

RoHS Directive 2015/863/EU of 31 March 2015

As well as with the requirements set out in the Laws of the United Kingdom relating to and applying the following standards:

Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment Regulations 2012 SI No. 3032 + 2019 SI No.492

In addition, all models are Certified to be in compliance with applicable requirements of UL 62368-1:2014, ANSI/AAMI ES60601-1:2005/AMD2 :2021, IEC 62368-1:2014 and IEC 60601-1:2005/A2:2020 including all EU national deviations, CAN/CSA C22.2 NO. 62368-1-14, CAN/CSA-C22.2 No.60601-1:14 , AM1:2014, AM2:2022, EN 62368-1:2014 and EN 60601-1:2006/A2:2021.

BY: John Thompson - President
John Thompson
PLACE: Integrated Power Designs
300 Stewart Road, Wilkes-Barre, PA 18706 USA
DATE: January 21, 2025

EUROPEAN CONTACT:
Compumess Elektronik GmbH
Lise-Meitner-Strasse 1
85716 Unterschleiβheim
Telephone (089) 32 15 01-0

UK CONTACT:
ALL PSU LTD
Laser Quay, Culpeper Close
Rochester Kent ME2 4HU
Tel : 01634 725527

CLASSIFICATION:
1. Protection against electric shock – Class I.
2. Protection against harmful ingress of water – IPXO (Non-protected), ordinary.
3. Methods of sterilization – None.
4. Suitability for use in an oxygen rich environment – End user responsibility, not evaluated.
5. Mode of operation – Continuous.

ENVIRONMENTAL: For Indoor Use Only.
No protective packaging required during transport.
Operating Temperature- 0-50°C
Storage Temperature- -40-85°C
Operating / Storage Humidity- 0-95%RH non-condensing
Operating Altitude- 3000m max.

INTEGRATED POWER DESIGNS

300 Stewart Road
Wilkes-Barre, PA 18706 USA
Phone: (570) 824-4666

Web: www.ipdpower.com
Email: sales@ipdpower.com
Fax: (570) 824-4843

WARNING! SHOCK HAZARD: Dangerous voltages are present on some components, printed circuit board traces and heatsinks.

WARNING! RISK OF FIRE: An open internal fuse indicates a catastrophic failure of circuit component(s). Repair must be by authorized IPD personnel only. Refer to fuse rating on power supply circuit board for rating.

WARNING! Modification of this equipment is prohibited without the authorization of the manufacturer.

SEPARATION: Primary to secondary creepage distance is 6.0mm minimum, clearance 3.2mm minimum (2MOPP). Primary to ground creepage distance is 2.0mm minimum, clearance 1.0mm minimum (1MOPP). Secondary to ground creepage is 2.3mm minimum, clearance 1.2mm minimum (Operational Insulation). The required separation must be maintained in the end use equipment to preserve the established means of protection.

OUTPUTS: The outputs are not acceptable for patient connection without additional isolation. All outputs are SELV under normal and single fault conditions unless otherwise indicated.

TEMPERATURES: The maximum operating temperatures of safety components as defined in the applicable safety standards must not be exceeded after installation in the end use equipment. Output power, ambient air temperature and convection or forced air cooling availability should be considered in the end use equipment.

HIPOT: In consideration of IEC 60601:2005 Clause 8.8.3, care must be taken to insure the voltage applied to a reinforced insulation does not overstress different types and levels of insulation. Breakdown of basic insulation and catastrophic failure of the power supply may result if a test voltage of greater than 1500 VAC is applied between primary and secondary circuits. Each isolating component is factory tested at 3000 VAC minimum prior to installation. Primary and secondary to ground capacitors may need to be disconnected prior to performing a dielectric strength test on the power supply or the end product.

INSTALLATION: The power supplies included in model listing on reverse side are considered components intended for professional installation into end use equipment. The protective earth (ground) terminal must be bonded to protective earth in the end use equipment.

CONNECTIONS / DIMENSIONS:

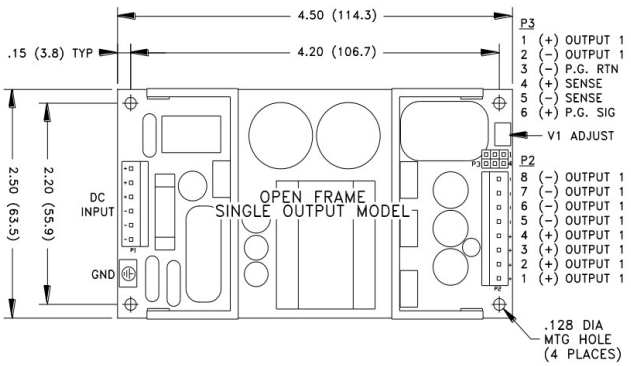

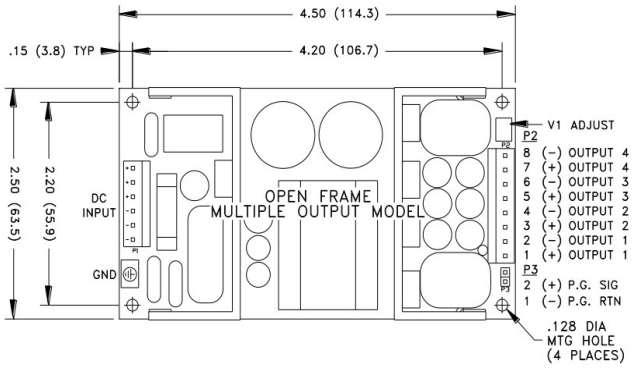

CONNECTORS:

P1: DC Input - .156 friction lock header mates with TE Connectivity 640250-6 or equiv. crimp terminal housing with TE Connectivity 3-640707-1 or equivalent crimp terminal

P2: DC Output (Single and Multiple) - .156 friction lock header mates with TE Connectivity 640250-8 or equivalent crimp terminal housing with TE Connectivity 3-640707-1 or equivalent crimp terminal.

G: Ground- .187 quick disconnect terminal.

P3: Power Good/Sense (Single) - .100 breakaway header mates with Molex 22-55-2061 or equivalent crimp terminal housing with Molex type 71851 or equivalent crimp terminal.

P3: Power Good (Multi) - .100 breakaway header mates with Molex 50-57-9002 or equiv. crimp terminal housing with Molex type 71851 or equiv. crimp terminal.